


Allura Xper Biplane FD20/10, 20/20

Preferred Room Layout

The layout shown below is based upon a typical equipment configuration with full movement range and should be considered as a general design guideline. Site conditions, application requirements, customer preferences, and/or equipment configuration may significantly impact suite design and equipment layout. It is recommended to request site-specific drawings from an Amber representative early in the design process.

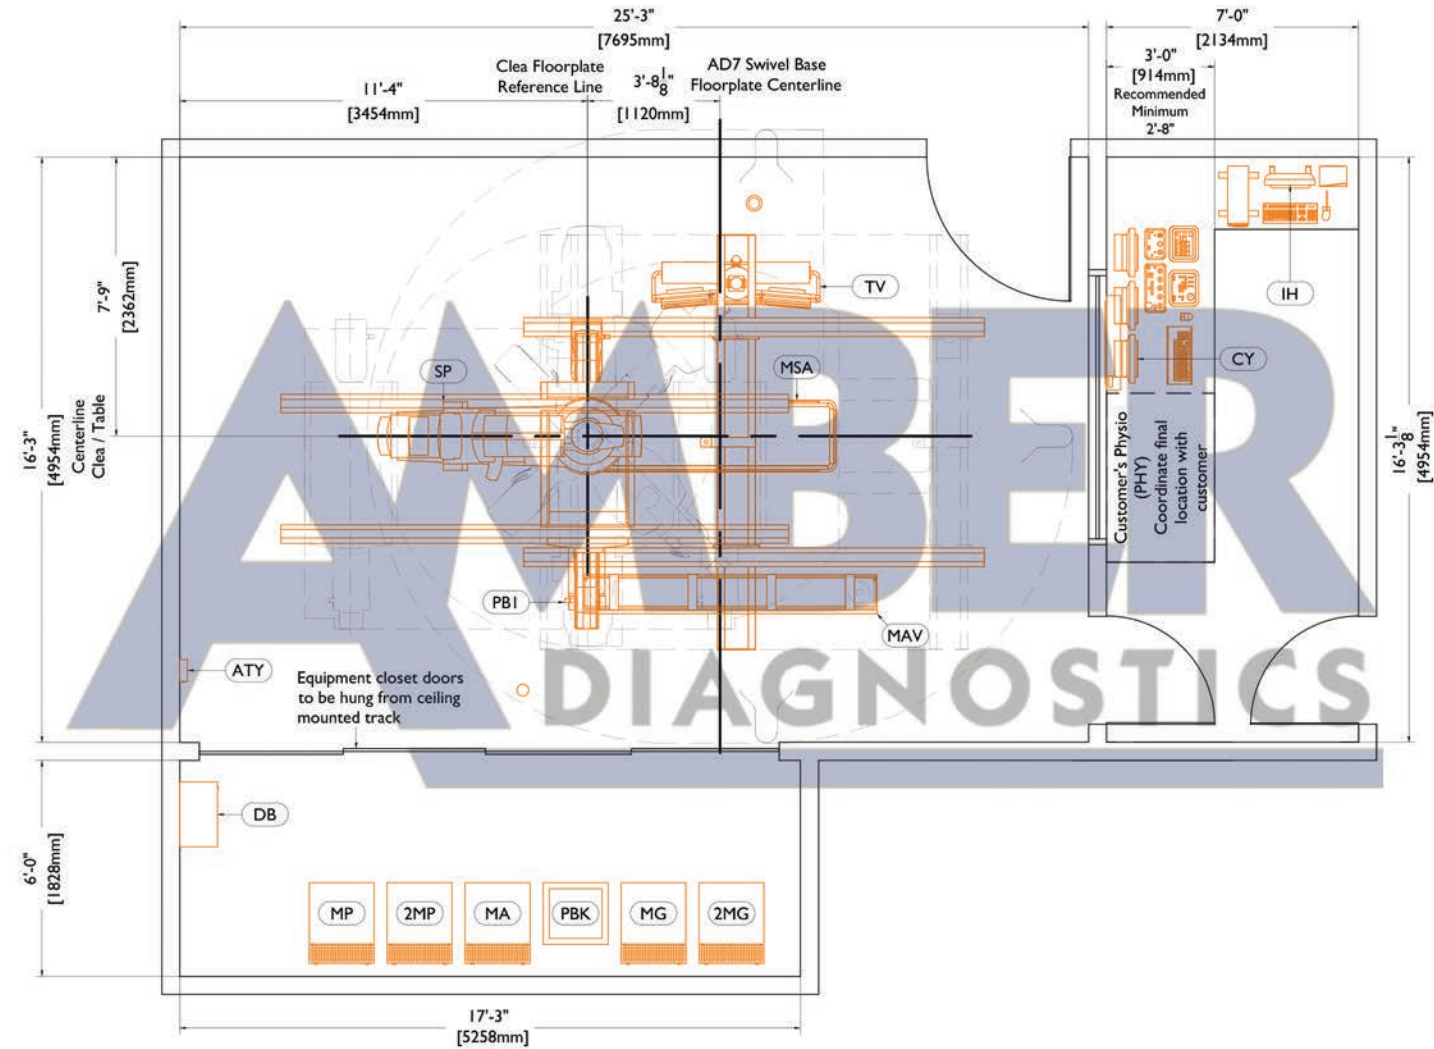

Equipment Layout

Required Ceiling Height: $9' - 9\frac{5}{16}'' + \frac{3}{16}'' / -0$ (2980mm, +4mm / -0)

Ceiling Height measured from top of Clea floorplate to bottom of Unistrut.

