


Allura Xper FD20 Ceiling

Preferred Room Layout

The layout shown below is based upon a typical equipment configuration with full movement range and should be considered as a general design guideline. Site conditions, application requirements, customer preferences, and/or equipment configuration may significantly impact suite design and equipment layout. It is recommended to request site-specific drawings from a Philips representative early in the design process.

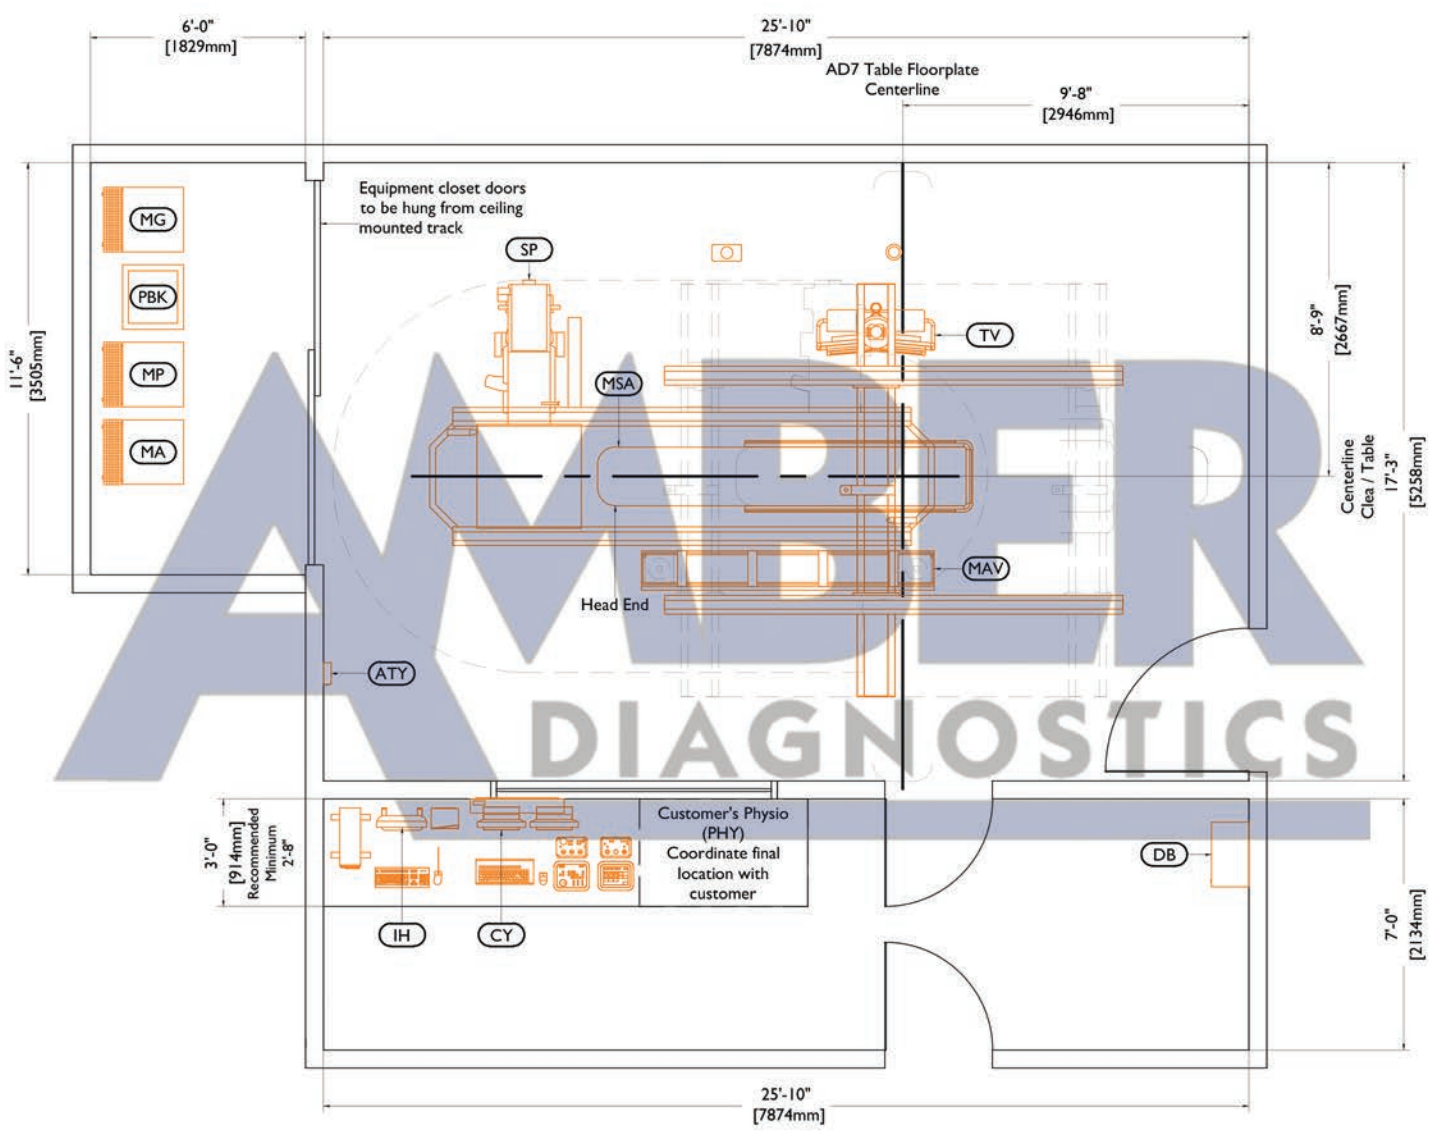

Equipment Layout

Required Ceiling Height : 9' - 6 ³/₁₆" , +³/₈ / -0
 (2900mm, +10mm / -0)

